


SWT= Threaded Switch Probes

mm [inch]

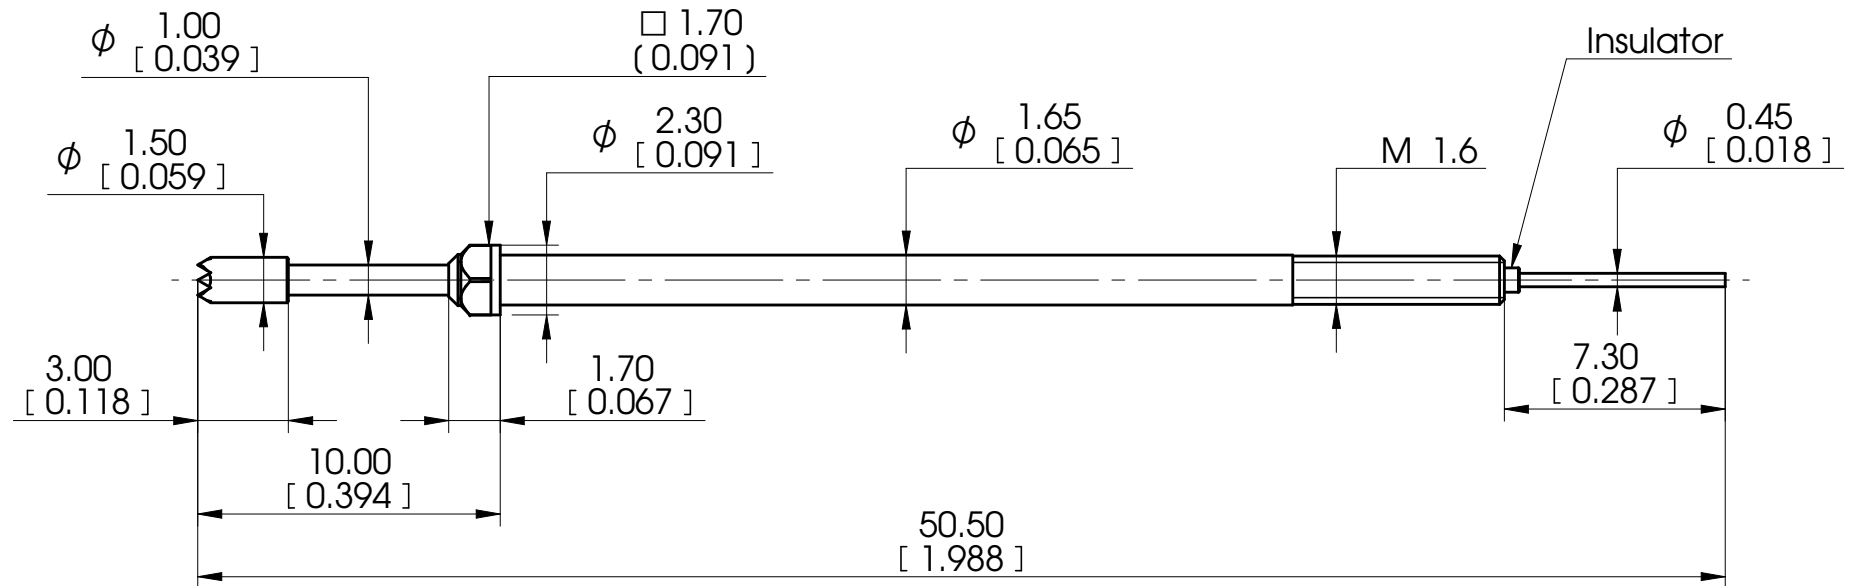

SWT1005 CG07 M

Minimum centers: 2.54 (.100)
 Full travel: 5.00 (.197)
 Working travel: 4.00 (.157)
 Switching path: 1.50 (.059) ± 0.20 (.008)
 Current rating: 3 A
 Probe resistance: < 30 mΩ
 Plunger material: BeCu - Gold Plated
 Barrel material: Brass - Gold Plated
 Spring material: MW - Plated

Operating temperature: -40 °C up to +80°C
 (-40 °F up to +176 °F)

Spring force at working stroke: 1.35 N (4.9 oz)


© COPYRIGHT 2023 EQUIP-TEST KFT. ALL RIGHTS RESERVED		Name	Date	Catalog Item: SWT1005 CG07 M			
	Designed	F.A	2023.04.14				
	Drawed						
	Checked						
This drawing, model, intellectual product belongs to Equip-Test Kft. Forwarding it to 3rd. party, copying it or using for any other purpose without the written approval of Equip-Test Kft., could entail to legal and criminal procedure!	Note				Drawing No.:		 TEST • SUPPORT • INNOVATE
						A4	



A4

SHEET 2 OF 1



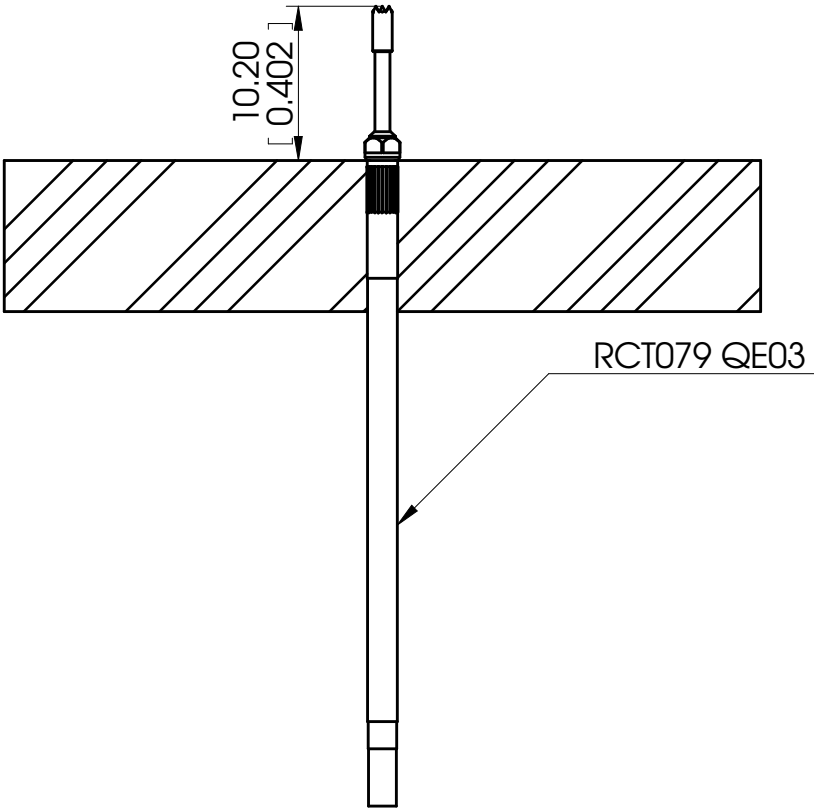

Tools for the Test Probe

- Tool Handle:
- TH3
- Adjustable Torque Handle:
- TTS01
- Insertion Bit:
- TBT10079
- Insertion/Extraction Bit:
- TBT10078

Tools for the Receptacle

- Tool Handle Insertion:
- TH1
- Tool Handle Insertion/Extraction:
- TH2
- Insertion Bit:
- TBR10036
- Extraction Bit:
- TBR10071

© COPYRIGHT 2023 EQUIP-TEST KFT. ALL RIGHTS RESERVED		Name	Date	Catalog Item: SWT1005 CG07 M		
	Designed	F.A	2023.04.14			
	Drawed					
	Checked					
This drawing, model, intellectual product belongs to Equip-Test Kft. Forwarding it to 3rd. party, copying it or using for any other purpose without the written approval of Equip-Test Kft., could entail to legal and criminal procedure!	Note	Drawing No.:			 TEST • SUPPORT • INNOVATE	
			A4	SHEET 2 OF 2		